



MycoFog® Biodecontamination System Model MF-1B Instrument User Manual

1

MycoFog® is an easy-to-use biodecontamination system designed to eliminate biocontaminants from incubators, gloveboxes and workstations used in cell culture and microbiology laboratories. The *MycoFog®* System comprises an instrument (*MycoFog®* biodecontamination fogger) and *MycoFog®* reagent pods or bottles with our proprietary H₂O₂ formulation.

Carefully read these operation and care instructions prior to first use.

Items required but not supplied: USB charger, 5V

Caution



Ensure incubator is clean* and in good working order, able to evenly achieve 37°C-45°C (this temperature range has been validated by *MycoFog®* and partners, the *MycoFog®* process may be effective at other temperatures but not yet validated by us) *The *MycoFog®* biodecontamination process complements cleaning but does not replace cleaning. Please consult your incubator operating manual for the manufacturer's cleaning protocol.

Operation

1. Charge *MycoFog®* biodecontamination fogger overnight using the provided USB cable (USB charger not supplied). Charge indicator light is on when charging, off when charge is complete.
2. Prepare incubator as noted in "Incubator Preparation" below.
3. Open *MycoFog®* biodecontamination fogger by twisting the upper cylinder counterclockwise and pulling it away from the clear base.
4. Pour contents of appropriate *MycoFog®* reagent bottle (<https://mycofog.com/product/mycofog-biodecontamination-reagent/>) into the center ring (reservoir) of the lower cylinder. Place the wick into the wick receptacle as noted in "Wick Replacement" below. Replace the wick holder.
5. Carefully place upper cylinder back onto lower cylinder of the *MycoFog®* biodecontamination fogger and twist clockwise to lock, taking care not to let reagent spill from center ring.
6. Place *MycoFog®* biodecontamination fogger in upper 1/3 of incubator as shown in "Incubator Preparation" below. Wait 5 minutes for wick to wet completely.
7. Press function button once. Observe fog emitted by device from *MycoFog®* biodecontamination fogger mist port (see diagram below).
8. Close and lock incubator, glovebox or workstation and place lab tape over door lock.
9. Set lab timer for 180 minutes. *MycoFog®* biodecontamination fogger will shut off automatically at the end of the vapor exposure cycle. If using alternate 37°C protocol, use a 4-hour cycle, set timer for 240 minutes. For incubators < 120 L chamber volume, extend 45°C protocol to 4 hours, extend 37°C protocol to 5 hours,
10. After 180 minutes (or 240 minutes), open incubator and remove *MycoFog®* biodecontamination fogger. Open the *MycoFog®* biodecontamination fogger and remove the used wick, as noted below, and discard. Rinse the reagent reservoir with distilled or laboratory DI water. Let dry before storing.
11. Incubator/glovebox/workstation is now ready to use, restart according to your laboratory procedure or instrument manual.

CAUTION

Use only *MycoFog* reagents in the *MycoFog®* biodecontamination fogger. Use of other reagents may harm device or result in inadequate decontamination.

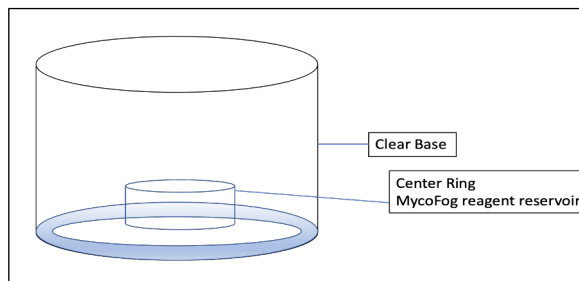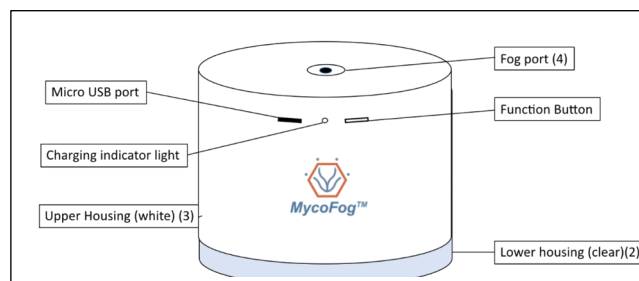

info@mycofog.com

415-298-5456

©MycoFog® 2024 All rights reserved

Rev 3.2



MycoFog® Biodecontamination System Model MF-1B Instrument User Manual


2

Function Button Operation

Use a short press on function button once to start the *MycoFog*® biodecontamination fogger, short press 2nd time pulses fog, 3rd time turns off.

The light will blink and turn off automatically when *MycoFog*® reagent is used up, indicating the end of the first step in the disinfection cycle. Long press turns light on, 2nd long press dims, 3rd long press turns light off.

WICK REPLACEMENT (cut-away view)

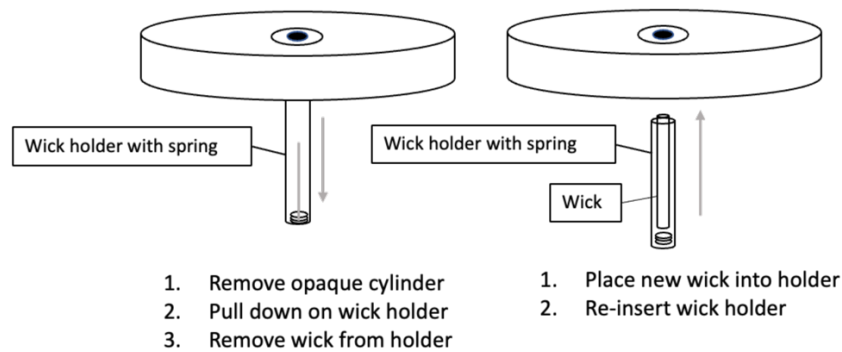

INCUBATOR PREPARATION:

1. Remove all cultures & labware from incubator.
2. Remove water from water pan.
3. Set incubator temperature to 37°C or 45°C.
4. Disable gas control.
5. Arrange shelves so that all shelves are in the lower ½ to 2/3 of the incubator.
 - a. If the incubator has a fan inside the chamber that does not use a HEPA filter, all shelves should be in the bottom ½ to 1/3 of the chamber
6. Place *MycoFog*® biodecontamination fogger on uppermost shelf.



TROUBLESHOOTING

1. If there is no spray emitted from the *MycoFog*® biodecontamination fogger spray port, turn off unit and wait 10 min for wick to completely wet with reagent.
2. *MycoFog*® biodecontamination fogger only operates right-side up. Keep level.
3. If the volume of spray is low (refer to www.mycofog.com/troubleshooting), the fogger element may be cleaned with vinegar and cotton swab.
4. If the volume of spray is low, the battery may be low. Recharge

| Product Name | MycoFog® Biodecontamination Fogger | Items included |
|------------------|------------------------------------|------------------------------------|
| Product Number | MF-1 | MycoFog® Biodecontamination Fogger |
| Dimensions | 130 diameter x 100 mm high | Manual |
| Materials | ABS+Polycarbonate | Additional wick |
| Power | 2W | USB cable |
| Battery Capacity | 2000 mAh | |
| Input/Output | DC 5F/0.8 A | |
| Battery Type | Lithium Ion | |
| Charger type | Micro USB | |
| Device Standard | GB4706.1-2005/GB4706.48-2009 | |

Warning: Use only *MycoFog*® reagents in this instrument. Use only as described in the user's manual. For Research Use Only, not for Diagnostic or Therapeutic Use. Use caution when using and storing lithium batteries.

Assembled in USA
www.mycofog.com

