

MycoFog® Quick Start Guide Please consult full manual at https://mycofog.com

Day before use: Charge MycoFog® Device with supplied cable.






> 8 hours

Day of use: Take out all cell cultures from incubator, set Incubator to 37 °C or 45°C, turn off gas control and remove water pan or turn off active humidification. The MycoFog® biodecontamination process complements cleaning but does not replace cleaning. Please consult your incubator operating manual for the manufacturer's cleaning protocol.

1. Open MycoFog®

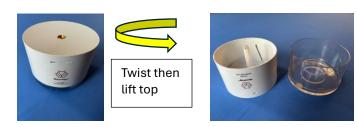

2. Pour MycoFog® Reagent into reagent reservoir of MycoFog®



Quick Start v 3.0.4

MycoFog® products are for Research Use Only, not for diagnostic or therapeutics use.



3. Remove the wick holder, insert wick, replace holder and press firmly. Replace top of MycoFog®.







4. Place MycoFog[®] in incubator, mid-chamber, wait 5 minutes.





5 minutes

5. Press Start



6. Close incubator door set timer.



180 Minutes (or **240** mins if using 37 °C)

7. Remove MycoFog®, if necessary return temperature to 37°C. Your Incubator is now decontaminated and ready for use!