



## MycоФog® Quick Start Guide

Please consult full manual at <https://mycofog.com>

**Day before use:** Charge MycoFog® Device with supplied cable.




> 8 hours

**Day of use:** Take out all cell cultures from incubator, set Incubator to **37°C** or **45°C**, turn off gas control and remove water pan or turn off active humidification.

**The MycoFog® biodecontamination process complements cleaning but does not replace cleaning. Please consult your incubator operating manual for the manufacturer's cleaning protocol.**

### 1. Open MycoFog®

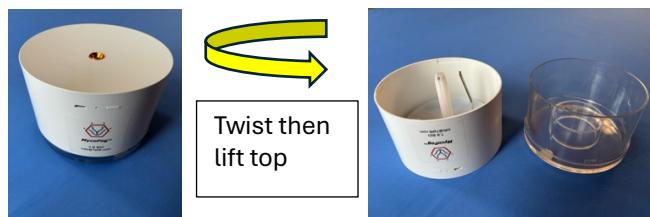

### 2. Pour MycoFog® Reagent into reagent reservoir of MycoFog®





**3.** Remove the wick holder, insert wick, replace holder and press firmly. Replace top of MycoFog®.



**4.** Place MycoFog® in incubator, mid-chamber, wait 5 minutes.



5 minutes

**5.** Press Start button for 2 seconds, indicator light will flash as described in manual.



**6.** Close incubator door set timer.

180 Minutes (or **240** mins if using 37 °C)

240 Minutes for incubators >500 L (or **300** min if using 37 °C)

**7.** Remove MycoFog®, if necessary return temperature to 37°C. Your Incubator is now decontaminated and ready for use!